

# AQUASOL DIGITAL

## BENCH TOP DO METER

### ABM404



Product Manual / Warranty Card

## Introduction

We thank you for having purchased bench top meter. Before using the instrument, please note that the operation instructions should be read carefully, which will help you to operate and maintain the instrument.


## Specification:

Model	ABM404 - Bench Top DO Meter		
Parameter	DO	O <sub>2</sub>	Temp
Range	0 to 20.00 mg/L	0 to 200.0 %	0 to 110 Deg C
Accuracy	2%	2%	±0.2
Resolution	0.01 mg/L	0.01	0.1 Deg C
Calibration	DO - O <sub>2</sub> Air Calibration (101.7 mg/l)		
ATC	Yes		
Output	USB Connectivity with Computer		
Stirrer	Magnetic Stirrer Provided		
Sensor	DO & Temperature sensors included. pH/ORP ( To be purchased extra)		

## Accessories:



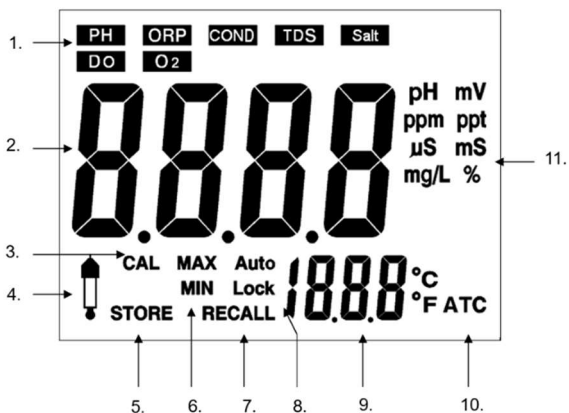


DO Sensor, Temp. Sensor, Standard Solution, Power Adapter,  
Electrode Holder with Magnetic Stirrer, USB Software.

## Display Details



1. Function Mode
2. Measuring Value
3. Calibration Mode
4. Calibration error indicator
5. Reading stored indicator
6. MAX & MIN Value
7. Recall Mode
8. Auto lock or manually lock current reading
9. Temperature Indicator
10. Auto Temperature Compensation
11. Unit

## Keyboard Details

	Single Press Lock the current reading, Press for 3 sec. to enter or exit MAX/MIN mode.
	Single Press to Store the current reading. Press 3 sec. to enter Recall mode.
	In Recall mode, browse records. Press both together 3 sec. to enter Advance Setting
	Single Press to Choose different Function mode. Press 3 sec. to switch °C/°F, or switch mg/L or ppm
	Turn on or off power. Press 3 sec. to enter calibration mode

## Magnetic Stirrer Operation

- 1) Connect AC adaptor with power source and Stirrer
- 2) Assemble the Electrode Holder and Stand with the Stirrer Base.
- 3) Place the Sample container with stirrer bar in center of stirrer.
- 4) Power On the Stirrer and Adjust Speed with Regulator

## Meter Preparation

- 1) Connect AC adaptor with power source.
- 2) Connect the DO and Temperature Electrode
- 3) Clean the Electrodes with DM Water and Power On the Meter

## DO Electrode Preparation

1. Take DO Electrode and remove the protection cap from the probe.
2. Now remove the membrane cap carefully without damaging the film.
3. Fill the membrane cap with the electrolyte solution up to the bottom of the threads on the inside of the cap. Tap the Cap to remove any air bubbles.
4. Now Fix the membrane cap back in such a way that no air bubble is present in the cap.
5. Press Power button to turn the meter power on.

## DO Calibration:

### Air Calibration

1. Power on the meter and remove the protection cap from the probe.
2. Keep the Electrode exposed to Air for some time.
3. Press **MODE** to choose **02** mode and wait 25 minutes to 30 minutes for the probe to polarize. The reading should be approx. 101.7% (saturation) after the probe has completely polarized.

4. Once the reading is 101.7%, Press and hold **CAL** for 3 sec. to enter calibration mode. The display will appear **CAL** and flashing 101.7%. When the display stops flashing and indicates “SA”, then “End” while calibration ends, and will return to measurement mode.

## Zero Calibration

To improve measurement accuracy for very low or very high DO readings.

Place the probe into a Zero Oxygen calibration solution (AMEB1DEO) and wait for stable 0% Reading. Stability in a zero solution may take many minutes, depending on probe history. Once 0% is press and hold **CAL** to enter calibration.

### Note:

1. Calibration error indicator icon will appear, and “Err” instead of “SA”, if calibration fails.
2. If the reading is not 0% while the probe is not connected, calibrate it in the air without probe to make reading becomes 0%.

## DO Measurement:

1. Confirm Calibration is Done.
2. Now select DO or O2 by pressing **MODE** on the meter.
3. Remove the protection cap & place the probe in the sample.
4. Stir the probe in the sample to remove any trapped air bubbles from the membrane surface.
5. Allow the meter time to settle and read the results.

## Note:

1. The larger the difference in temperature between the probe and the solution the longer it will take for the reading to stabilize.
2. Cover the probe with the probe cap. The sponge contained in the cap should be moistened (not soaked) with DI (distilled water) or clean tap water.

## MAX/MIN mode:

Press and hold **MAX/MIN** button until the display appears flashing MAX and MIN icons to enter MAX/MIN. Press **MAX/MIN** lightly to browse MAX and MIN value during this mode. To exit this mode, press and hold **MAX/MIN** button again until the flashing MAX and MIN icons disappear and return to measuring mode.

## Store and Recall mode:

In measuring mode, press **STO** to store the current reading. The Store icon and the ordinal of this record will appear on the display.

Press and hold **RCL** for 3 sec. to enter Recall mode. In this mode, use ▲ or ▼ to browse records. Press and hold **STO** to exit this mode and return to measuring mode.

In Recall mode, press ▲▼ together for 3 sec. to clean all the records in the memory.

## Advanced Setting:

In DO measuring mode, press ▲▼ together for 3 sec. will enter advanced setting.

Press **STO** to set Salt Compensation and use ▲▼ to set from 0 to 50 ppt.

Then press **MODE** to confirm and return to measuring mode.

Press **LOCK** to set Altitude Compensation and use ▲▼ to set from 0 to 20K ft.

Then press **MODE** to confirm and return to measuring mode.

## Note:

Press **LOCK** to turn on or off “Auto Lock” function. Use ▲▼ to choose.

Then press **MODE** to confirm and return to measuring mode.


In advanced settings, press **CAL** to reset all settings to factory setting.

## Membrane Cap Replacement:

1. Do not touch the membrane as skin oils will interfere with the oxygen permeability rate of the membrane. Replace the cap carefully.
2. It is recommended that the probe remain attached to the meter during this replacement process.
3. Unscrew the cap firmly and carefully from the probe.
4. Rinse the old electrolyte solution from the Cathode and Anode.
5. Use the supplied Polishing Strips to clean, polish, shine, and/or remove scratches from the cathode. Be sure to moisten the cloth before polishing the cathode. Do not over-polish the sensitive gold cathode.
6. Set the new replacement membrane cap on a flat surface. Leave the cap in this position during the replacement process.
7. Fill the membrane cap with the electrolyte solution up to the bottom of the threads on the inside of the cap.
8. Tap the membrane cap to release and prevent air bubble in electrolyte solution.
9. Keeping the cap in a fixed position on a flat surface, carefully insert the probe into the new cap by first dipping and removing the probe several times from the cap. With each dip, push the probe progressively deeper into the bonded cap. Finally, screw the probe slowly onto the cap until fully tightened. The dipping and removal technique minimizes the

introduction of air bubbles into the electrolyte solution. Air bubbles in the electrolyte can affect measurements.

10. It is normal that excess electrolyte solution will leak out the cap during this replacement since it minimizes the introduction of air pockets. Clean off the excess electrolyte before use.

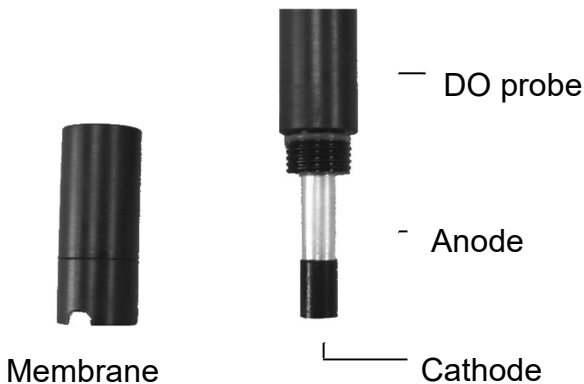

## DO probe clean:

When the Do reading is unstable or incorrect, please follow the below steps to clean the probe.

1. Unscrew the membrane cap from the probe.
2. Put the sand paper on the table, let the coarse side on the up side, and add some water on it.
3. Rub the cathode part against the sand paper according to figure "8" for around 10 times.
4. Use the sand paper to clean the anode part.
5. After cleaning the probe, please refill new electrolyte into the membrane cap.



## Connect to PC:

OS: Windows7 or Above. Connect Cable to USB Port.

## Software Installation


Download the Software from - [bit.ly/4rfVXQ3](http://bit.ly/4rfVXQ3)

Unzip the File Driver folder. Install Drivers and then install "ADB400\_APP.exe"


## Software Operation

Double-click "ADB400\_APP.exe" to start the program.

Click **Setting** button to set COM port in the Setup window.

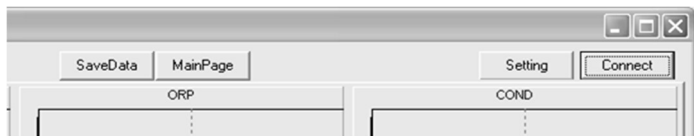


Choose the responding Port and then click **OK**.

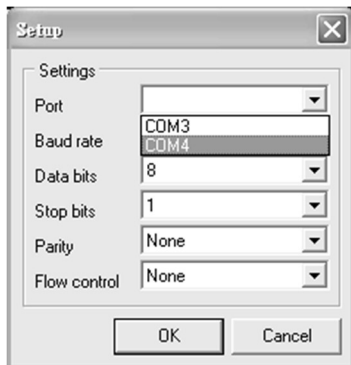

Fill in desired measuring interval seconds, and click **set**.




Click **Connect** to get readings and draw the curve.

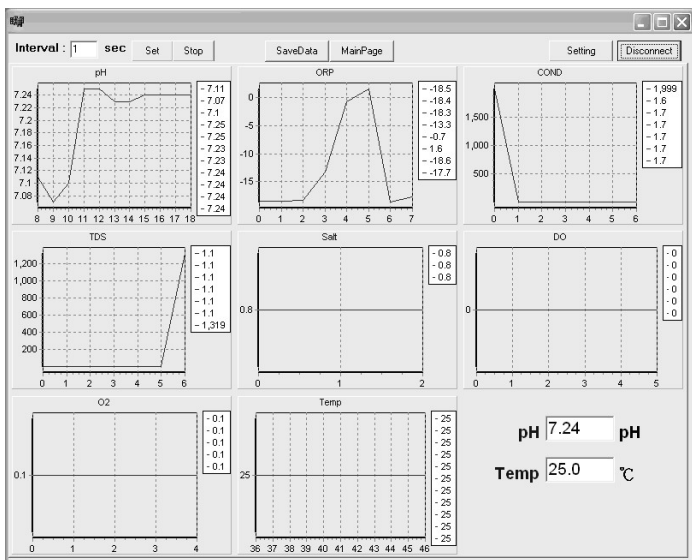

Click the small graphs of each mode in the main window can enter a big window with detail reading information. Click **MainPage** to back to the main window.

In each big window, click **SaveResult** will export the readings to .txt file.

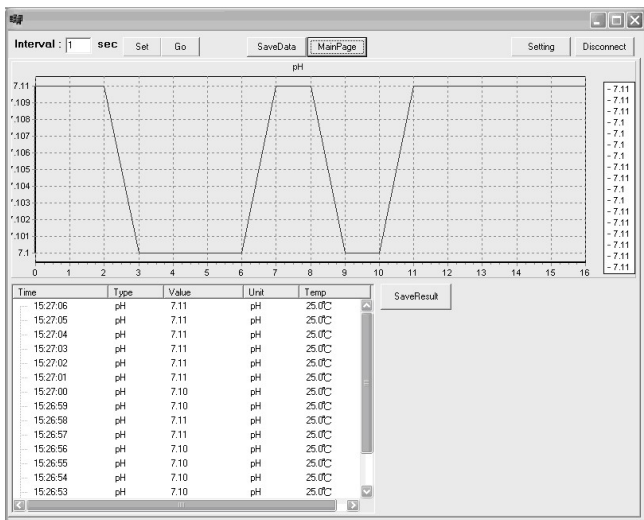

Click **SaveData** and then press and hold **RCL** to enter Recall mode.

Press **MODE** to export all the records to the program.

The records can also be saved as a .txt file by clicking **Save Result**

Interval : 1 sec Set Go SaveData MainPage Setting Disconnect

DataNo	Type	Value	Unit	Temp	TempUnit
1	ORP	0.7	mV		
2	ORP	0.7	mV		
3	ORP	0.8	mV		
4	pH	0.7	mV	77	°F
5	pH	0.7	mV	77	°F
6	pH	0.7	mV	77	°F
7	TDS	1319	ppm	77	°F
14	DO	8.38	mg/L	25	°C
15	DO	8.38	mg/L	25	°C
16	DO	8.38	mg/L	25	°C
17	O2	11.6	%	25	°C
18	O2	11.6	%	25	°C
19	O2	11.6	%	25	°C
20	O2	11.6	%	25	°C
21	pH	7.10	pH	25	°C
22	pH	7.10	pH	25	°C
23	pH	7.10	pH	25	°C
24	pH	7.10	pH	25	°C
25	TDS	0.9	ppm	25	°C

SaveResult

Note:

Please click **Disconnect** or close the program before turn off power or remove the USB cable.

# WARRANTY CARD

## Customer Details:

Name: \_\_\_\_\_

Address: \_\_\_\_\_

\_\_\_\_\_

Email Id: \_\_\_\_\_

Contact No: \_\_\_\_\_

## Dealer Details:

Name: \_\_\_\_\_

Stamp & Signature

## Product Details:

Bill No: \_\_\_\_\_ Bill Date: \_\_\_\_\_

Product Serial No: \_\_\_\_\_

Manufactured By



Rakiro Biotech Systems Pvt Ltd

[www.rakiro.net](http://www.rakiro.net)